

USER MANUAL

OAKWORKS® DTPM 300 Imaging Table



© Copyright 2010
OAKWORKS® Medical Equipment,
a division of OAKWORKS®, Inc.

This manual was originally drafted and approved in the English language.

Printed in U.S.A.

All rights are reserved. No part of this document may be photocopied, reproduced or translated to another language without prior written consent of OAKWORKS® Medical Equipment, a division of OAKWORKS®, Inc.

OAKWORKS® is a registered trademark of OAKWORKS®, Inc.

Notice

The information contained in this document is subject to change without notice and should not be construed as a commitment by OAKWORKS®, Inc.

OAKWORKS®, Inc. assumes no responsibility for any errors that may appear in this document nor does it make expressed or implied warranty of any kind with regard to this material, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

OAKWORKS®, Inc. shall not be liable for incidental or consequential damages in connection with or arising out of the furnishing, performance, or use of this document and the program material which it describes.

TABLE OF CONTENTS

Product Use Description	1
Contradictions	1
Important Safety Instructions	
Symbol Identification	1
Safety Instructions	2-3
Product Description & Photo	
DTPM300 - Polycarbonate Top.....	4
Installation	
Grounding	5
Directions for Use	
Foot Control Operations	6
Hand Control Operations	7
Manual Longitudinal Travel Operation	8
Patient Restraint Strap	8
Top Pad Removal	9
Emergency Stop Use	9
Carbon Fiber Arm Board	10
Fluoro Extender	10
Spine Positioning System II.....	11
Locking Casters Use.....	11
Reference	
Usable Imaging Area Diagrams	12-13
Cleaning & Disinfection	14
Inspections & Maintenance	14
Warranty Information	14
Model Number & Serial Number	15
Specifications	
Product Specifications	16
Environmental Conditions	16
Electrical Specifications	16
Guidance and manufacturer's declaration - Electromagnetic emissions	17
Recommended separation distances	17
Guidance and manufacturer's declaration - Electromagnetic immunity	18-19
Contact Information	back cover

PRODUCT USE DESCRIPTION / IMPORTANT SAFETY INSTRUCTIONS

PRODUCT USE DESCRIPTION

The Oakworks® Fluoroscopy table with Trendelenburg feature is a radiographic table intended for use with mobile or compact stationary C-arm Fluoroscopy Systems where the x-ray generator is located below the table top. It is ideally suited for pain management imaging and therapeutic procedures. It is suitable to use for diagnostic x-ray imaging and imaging during therapeutic procedures such as spinal injections, vertebroplasty procedures and other pain management procedures.

It is intended to be operated by a healthcare professional in a medical environment. No special training is required but a review of the following Safety Instructions is important for the safety of the operator and patient. The healthcare professional should read and understand this entire manual before use with a patient.

Contradictions

The Oakworks® Fluoroscopy Table should not be used with Fluoroscopy systems having intensifier screens or film cassettes larger than 12 inches (30 cm) when an oblique angle of view is being used.

The table is not designed for and should not be used with Magnetic Resonance Imaging procedures.

Although the table accommodates a number of procedures, it is not intended to serve as a surgical procedure table.

SYMBOL IDENTIFICATION



This symbol, when used in this manual and on product labels, represents a caution warning. Be sure to read and comply with all precautions and warnings.



This symbol, when used in this manual and on product labels, warns against an electrical shock hazard. Be sure to observe and comply with all warnings.



This symbol, when used in this manual and on product labels, indicates the potential of exposure to harmful x-rays. Be sure to read and comply with all warnings.



This symbol, when used in this manual and on product labels, indicates that the table and components are a Type B Applied Part pursuant to IEC 60601-1: 2005.



This symbol, when used in this manual or on product labels, indicates a Protective Earth (Ground) Terminal.



This symbol, when used in this manual or on product labels, indicates the date of manufacture of the device.



This symbol, when used in this manual or on product labels, indicates alternating current (AC).



This symbol, when used in this manual or on product labels, indicates direct current (DC).



This symbol is used to indicate that the operator should consult the user manual.

IMPORTANT SAFETY INSTRUCTIONS

IMPORTANT SAFETY INSTRUCTIONS



CAUTION

READ AND SAVE THESE INSTRUCTIONS

Improper use of this device can cause injury. Be sure to read all operating instructions prior to use.

Duty Cycle: Max. 10% or 2 min. continuous use at full load then 18 min. without use.

Use caution when changing the table position to avoid collision with other moving or stationary items.

The Foot control must remain on the floor. Damage to the table will result if the foot control is placed under the column.

Medical Electrical Equipment needs special precautions regarding EMC and needs to be installed and put into service according to the EMC information provided in this manual.

Portable and mobile RF communications equipment can affect Medical Electrical Equipment.

The use of accessories, transducers, and cables other than those specified by the manufacturer, may result in increased Emissions or decreased Immunity of the table.

The table should not be used adjacent to or stacked with other equipment. If adjacent or stacked use is necessary, the Table should be observed to verify normal operation in the configuration in which it will be used.

The Imaging Table is designed to be a standalone table used with radiographic equipment. This table must not be modified or incorporated into any other equipment.

Weight limit (patient and accessories): 450 lbs. / 205 kg.

A pinch hazard exists under the side rail on either side of the table. The tabletop slides in a head to toe direction on a roller track system. Be sure to keep fingers and arms away from the table's slide mechanism.

The table top slide mechanism must be locked at all times except when the top is being moved. Both locking knobs must be securely tightened at all times - Travel can occur if the locking knobs are not secured by inadvertently pushing on the end of the table or by tilting the table.

The table utilizes four locking casters to permit movement of the table within the imaging suite. Accidental movement of the table may occur. Lock at least two casters prior to accomplishing imaging of the patient.

When lowering the table or using the Trendelenburg functions, make sure there is nothing underneath the table top that can impede motion (like stools, cabinets, accessory parts, cleaners, etc.)

Be certain that the table is completely lowered without any tilt being present prior to discharging an ambulatory patient. The patient may lose balance and fall.

The table is not to be used as a gurney or to move patients from room to room.

This table is not suitable for use in the presence of flammable anesthetic mixture with air or oxygen or nitrous oxide.

After unpacking your table, inspect it thoroughly for damage. If you suspect a problem, do not use the table and call our customer service department at 717.235.6807.



WARNING

Grounding reliability can only be achieved when this equipment is connected to an equivalent 3 prong receptacle marked "Hospital Only" or "Hospital Grade". See the Grounding section of this manual.

Patient must be secured with a Safety Restraint Strap prior to using the table.

Electrical Shock Hazard. The power supply/control module is located on the base of the table. No user serviceable parts are inside the control box. Refer servicing to qualified personnel. Unplug wall connector prior to contact with any cables connected to the power supply.

IMPORTANT SAFETY INSTRUCTIONS

WARNING

To reduce the risk of burns, fire, electric shock or injury to persons:

1. Unplug this furnishing from the electrical outlet before cleaning.
2. Unplug from outlet before adding or removing parts.
3. Never operate this furnishing if it has a damaged cord or plug, if it is not working properly, if it has been dropped or damaged, or dropped into water. Contact Oakworks Customer Service before use.
4. Keep the cord away from heated surfaces.
5. Never drop or insert any object into any opening.
6. Do not use outdoors.
7. Do not operate where aerosol (spray) products are being used or where oxygen is being administered.


DANGER

The potential of exposure to harmful x-rays exists when this table is in use. The use of adequate x-ray barrier devices is necessary to provide protection to both the operator and the patient. X-ray barrier devices are recommended for the patient outside of the intended target area to prevent exposure to scattered radiation from the x-ray generating source.

- OAKWORKS[®] Imaging Tables may be used for x-ray imaging where the x-ray generator is located below the tabletop and the image receptor is located above the tabletop. This is the recommended method. The tables may also be used for x-ray imaging where the x-ray generator is located above the tabletop and the image receptor is located below the tabletop. This application will result in greater patient exposure to x-rays. The operator must weigh this issue with the imaging requirements and patient exposure issues.
- The Imaging Tables may be used with the x-ray generator above the tabletop and a film cassette located on the tabletop. (See contradictions regarding film cassette size.)
- The x-ray generator should never be located above the tabletop when the OAKWORKS[®] Imaging Table and the OAKWORKS[®] Spine Positioning System/Prone Pillow are used together. This type of use requires that the x-ray generator is located below the tabletop and the imaging intensifier or film cassette located above the tabletop.

PRODUCT DESCRIPTION

DTPM300 Polycarbonate Top

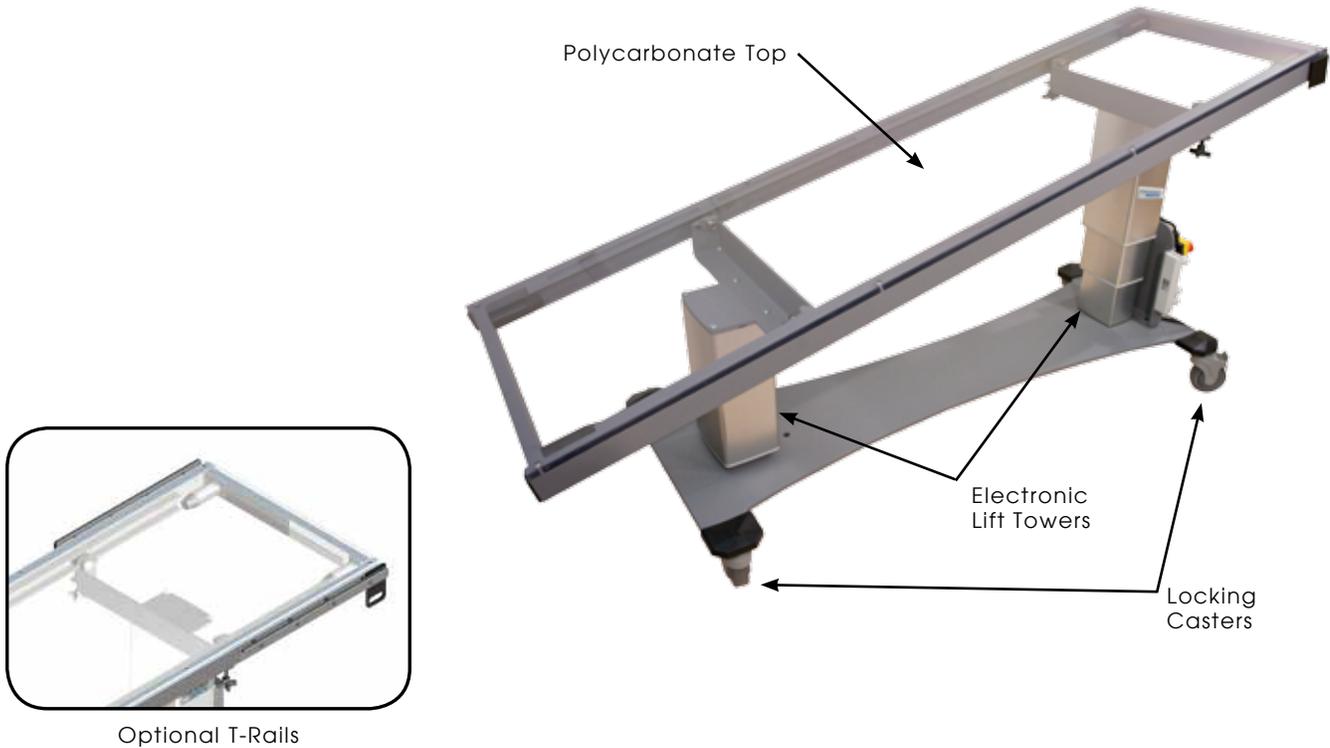

STANDARD SPECIFICATIONS	
Motion 1	Powered 24"-40" (61-101 cm.) Height Range
Motion 2	Powered $\pm 14^\circ$ Trendelenburg/ Reverse Trendelenburg
Motion 3	Manual 23" (58 cm.) Overall Longitudinal travel
Table Controls	(1) Foot Control & (1) Hand Control
Table Voltage Options	120V/60Hz or 230V/50Hz
Table Capacity	450 lbs. (205 kg.) (patient and accessories)
Polycarbonate Top	78" (198 cm.) Long x 24" (61 cm.) Wide
4" (10 cm.) Locking Casters	Locking / Unlocking Casters for mobile or permanent positioning
Patient Restraint Strap	Must be used during all procedures
Padding	1" (2.5 cm.) Comfort Foam™
Upholstery	Terra Touch™
Table Weight	390 lbs. (177 kg.)
Warranty	4 year parts, 1 year labor
Safety Listings	FDA, cETLus, CE marked

OPTIONS
5" (12.5 cm.) Locking Casters
6", 20", 78" (15.3 cm, 50.8 cm, 198.1 cm) or custom T-Rails Lengths
ACCESSORIES
Carbon Fiber Arm Board (Standard or Wide)
Spine Positioning System II
2" (5cm.) Tabletop Pad
Fluoro Extender

For electrical specs, see Specifications section.

INSTALLATION

The Imaging tables come completely assembled and ready to use. Plug the cord into a functioning outlet that is rated for the table. (see Grounding below)

Arrange the power cord and control cords so that they will not create a tripping hazard and where the controls are located to your liking and are conveniently accessible.

Be sure access to plug is not blocked for disconnecting the table from power.


GROUNDING



DANGER

Risk of Electric Shock - Connect this furnishing to a properly grounded outlet only.

This product must be grounded. If it should malfunction or break down, grounding provides a path of least resistance for electrical current to reduce the risk of electric shock. This product is equipped with a cord having an equipment-grounding conductor and a grounding pin. The pin must be plugged into an appropriate outlet that is properly installed and grounded in accordance with all local codes and ordinances. See U.S. sample below.

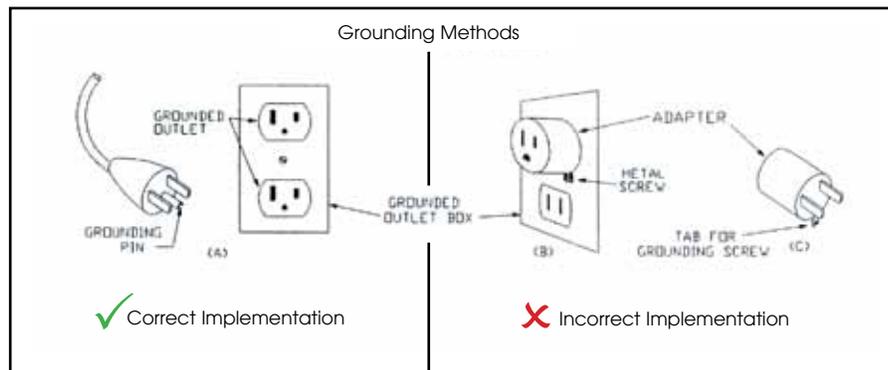

Improper connection of the equipment-grounding conductor can result in a risk of electric shock. Check with a qualified electrician or service person if you are in doubt as to whether the product is properly grounded. Do not modify the plug provided with the product - if it will not fit the outlet; have a proper outlet installed by a qualified electrician.

DIRECTIONS FOR USE

The Oakworks® Fluoroscopy Table with Trendelenburg positioning offers a variety of positioning capabilities for diagnostic x-ray imaging and imaging during therapeutic procedures.

DANGER

Should the use of this device create a circumstance under which the patient could be overexposed to ionizing radiation, discontinue use immediately and determine an alternative radiology table or alternative x-ray generating source to use.


FOOT CONTROL OPERATIONS

CAUTION

The Foot control must remain on the floor. Damage to the table will result if the foot control is placed under the column. When operating the table's controls, be sure to observe all cautions and warnings.

All Oakworks® Fluoroscopy Tables come complete with one foot control to control height and a hand control to operate the height and trendelenburg functions of the table.

Operate the Foot control as shown below to raise or lower the height of the table. To increase or decrease the angle of tilt up to a maximum of 14° on either side, see the Hand Control Operations on the next page.

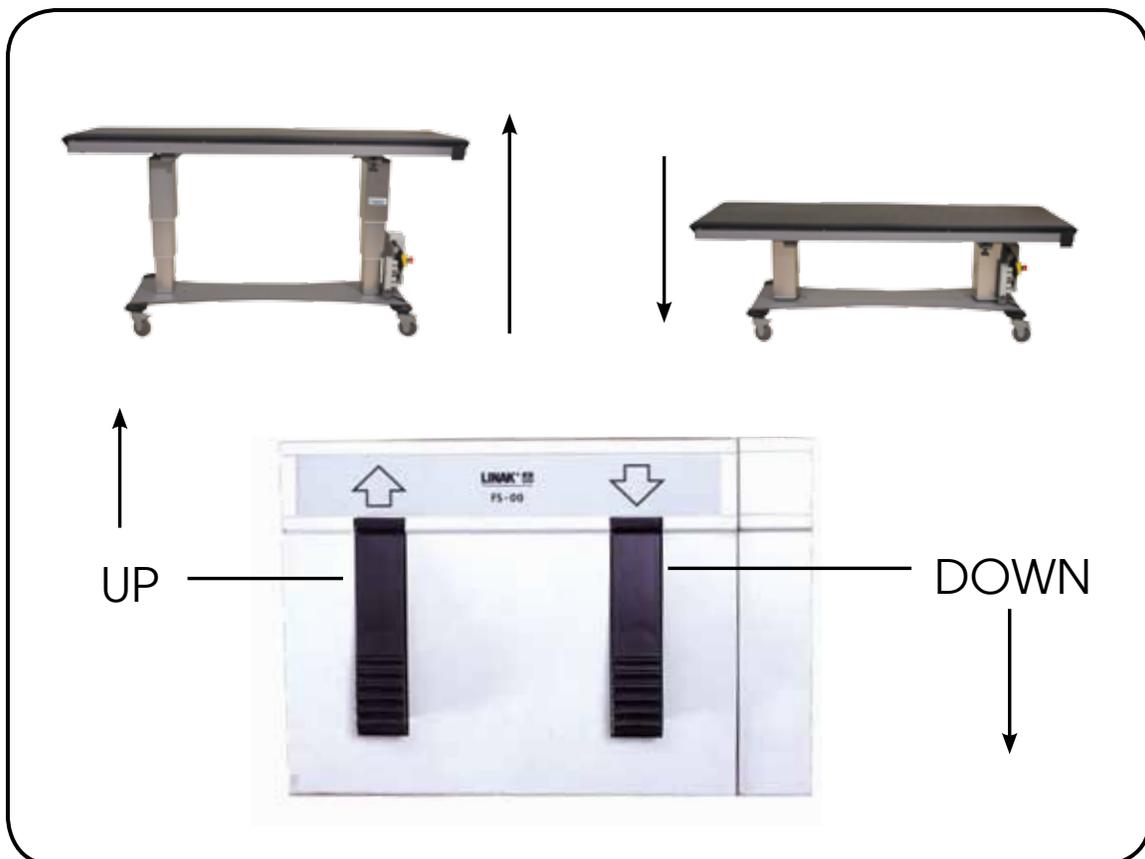

DIRECTIONS FOR USE

HAND CONTROL OPERATIONS



CAUTION

When lowering the chair or using the Trendelenburg functions, make sure there is nothing that can impede motion (like stools, cabinets, accessory parts, cleaners, etc.) When operating the table's controls, be sure to observe all cautions and warnings.



Reverse Trendelenburg:

- activates tilt up to 14°
- positioning stops when table is level; press again for complete reverse.



Trendelenburg:

- activates tilt up to 14°
- positioning stops when table is level; press again for complete reverse.



Height Up:

- Elevates table top
- Trendelenburg / Reverse Trendelenburg positioning are preserved during elevation



Height Down:

- Lowers table top
- Trendelenburg / Reverse Trendelenburg positioning are preserved during lowering

DIRECTIONS FOR USE

MANUAL LONGITUDINAL TRAVEL OPERATION



CAUTION

When operating the table's locking knob be sure to avoid pinching. Keep your fingers and other materials clear from the pinch point. Both locking knobs must be securely tightened at all times - Travel can occur if the locking knobs are not secured by inadvertently pushing on the end of the table or by tilting the table.

The table is designed to allow travel in either the left or the right direction as shown. This feature should only be used when the table is level.



LOCKING KNOB OPERATION

A Locking Knob is provided on each side of the table just under the side rail.

Rotate the locking knob several turns counter-clockwise to loosen. Slide the table in the desired direction. Rotate the locking knob clockwise until tight to secure the table against traveling.



PATIENT RESTRAINT STRAP




CAUTION

The Patient Restraint Strap must be used during all procedures to prevent the patient from falling off the table.

The strap has Velcro® attached to the ends. The Strap is attached as follows:

1. Place the center of the strap around the patient's waist. Relocate the strap as necessary for adequate clearance.
2. Take the ends of the strap down around the tabletop. Pull the strap snug underneath the table and press the two Velcro® ends together.
3. Check the strap to assure adequate patient restraint prior to using the Trendelenburg functions.

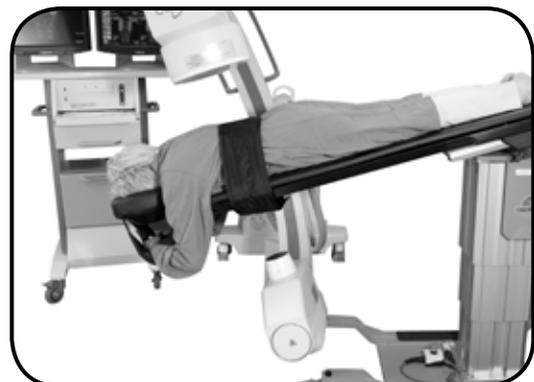

DIRECTIONS FOR USE

TOP PAD REMOVAL


Remove the Top Pad by pulling the flaps at the underside of the table on either end until the Velcro® detaches. Replace the pad by first centering on the table and then pressing the flaps in place, anchoring the flaps to the Fastener Velcro® as shown. (applies to both the 1" (2.5 cm.) & 2" (5 cm.) pads)

Underside of Tabletop



EMERGENCY STOP

All electric tables are equipped with an emergency stop switch.

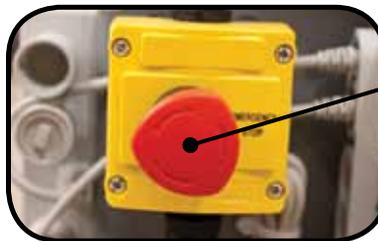

If necessary, you can also remove the plug from the outlet. Be sure access is not blocked for disconnecting the table from power.

DIRECTIONS FOR USE

CARBON FIBER ARM BOARD (ACCESSORY)



CAUTION

Do not place undue weight or downward pressure on the Carbon Fiber Arm Board. It is a positioning device for the arms and should not be used as leverage to get on or off the table. Injury can occur. DO NOT exceed 30 lbs. (13.6 kg) of load on the **Support Section**. Injury can occur.

Use

This radiolucent device can be used with any flat support surface where ionizing radiation (x-ray) is utilized for imaging. It can be used to support arms and feet.

Directions

Unfold the Arm Board and slide the **Base Section** under the patient and the table pad. Position the patient and the **Support Section** to suit the needs of the procedure. The weight of the patient will hold the Arm Board in place.


Rotate the **Support Section** to the desired position. This section rotates up to 180°.



Prone Position at 135°



Supine Position at 180°

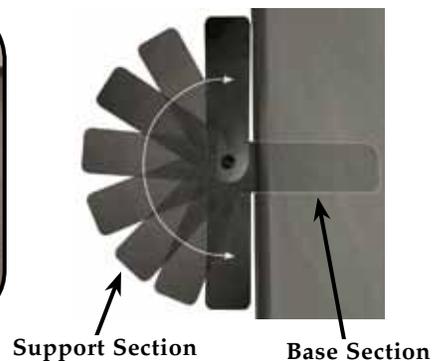

Support Section

Base Section

To remove the Arm Board, ask the patient to move their limb off the **Support Section** and lift their body slightly. This will allow you to pull out the base section of the Arm Board.

Fold the **Base and Support sections** for storage.

FLURO EXTENDER (ACCESSORY)



CAUTION

Do not place undue weight or downward pressure on the Fluoro Extender. It is a positioning device for the arms and should not be used as leverage to get on or off the table. Injury can occur.

The Oakworks® Fluoro Extender is radiolucent and offers extra width only where you need it for greater positioning accuracy with optimum imaging. The Fluoro Extender is inserted under the table top pad.



DIRECTIONS FOR USE

SPINE POSITIONING SYSTEM II (ACCESSORY)

For directions on the use of the Spine Positioning System, see publication "Spine Positioning System"
Part number MMMMNUP0003



LOCKING CASTERS USE

All four casters should be locked at all times during use with a patient.



LOCKING THE CASTERS

1. Place your shoe on the end of the casters locking tab.
2. Press firmly downward until you here a clicking noise and the caster is locked.




UN-LOCKING THE CASTERS

1. Place your shoe on top of the casters locking tab.
2. Press firmly inward and downward until you here a clicking noise and the caster is unlocked.


REFERENCE

USABLE IMAGING AREA


CENTERED FOR A-P VIEW:

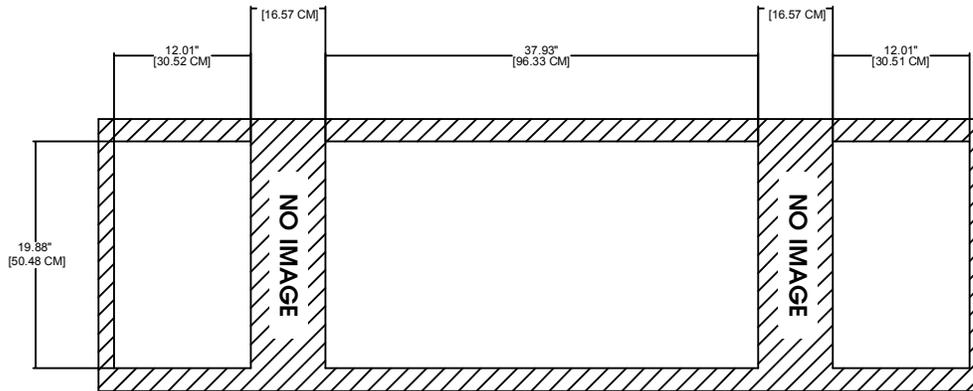

CENTERED OBLIQUE 30° VIEW FROM VERTICAL

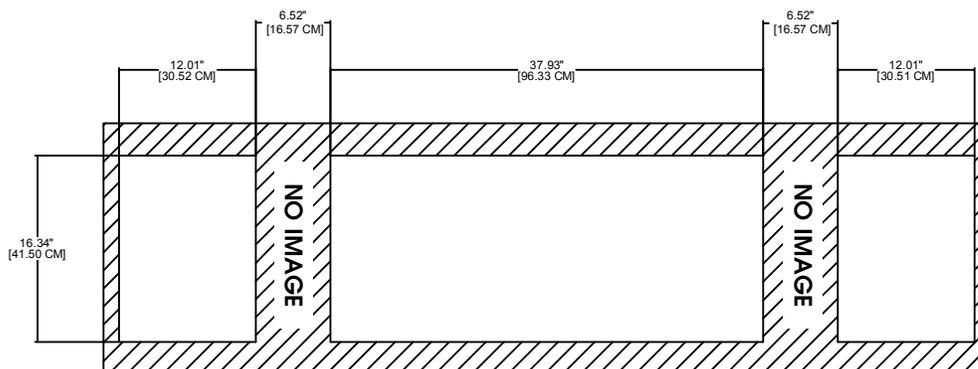


CENTERED CAUDAL 30° VIEW FROM VERTICAL

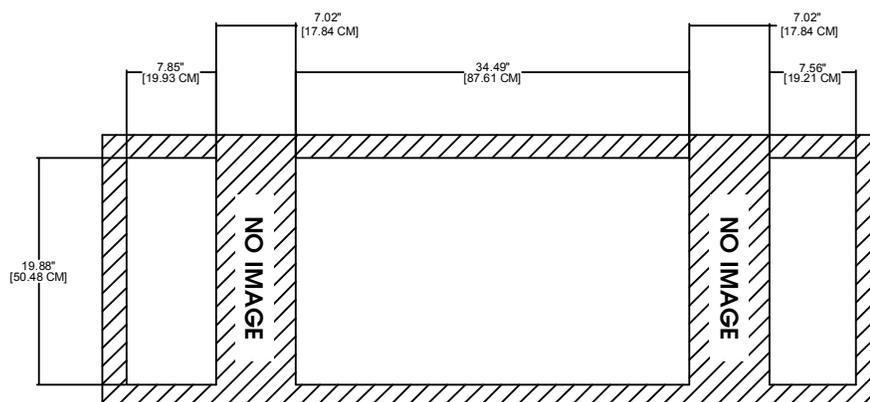


REFERENCE

OFFSET FOR A-P VIEW:

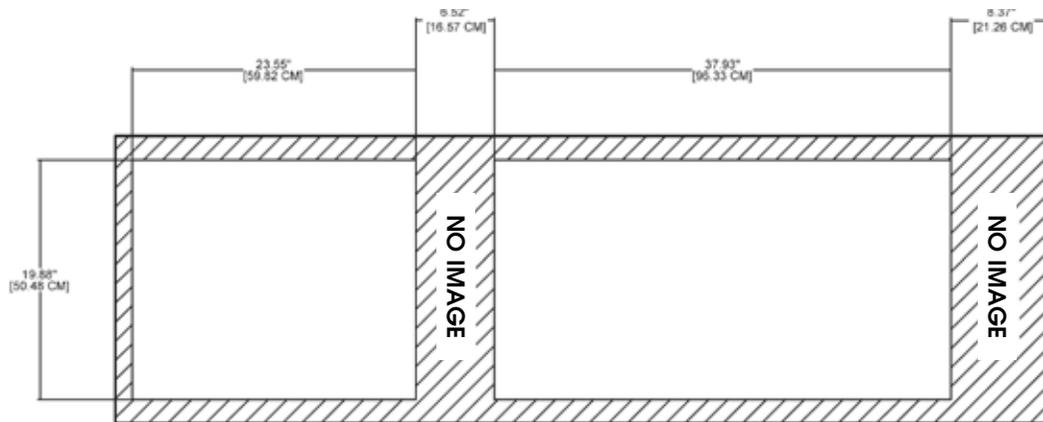

OFFSET CAUDAL 30° VIEW FROM VERTICAL

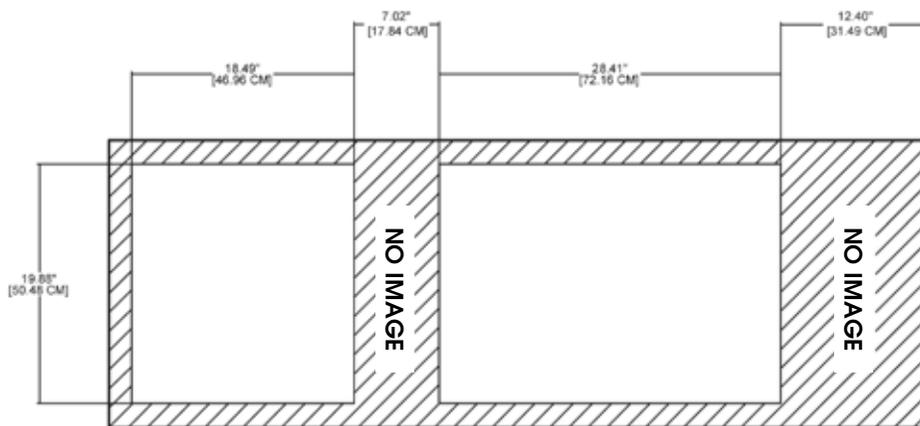

CLEANING & DISINFECTION / INSPECTIONS / WARRANTY

CLEANING & DISINFECTION



WARNING

Before cleaning with any liquid cleaner be sure to unplug the power cord from the outlet.

Use a 10% sodium hypochlorite (bleach) solution or *Recommended Disinfectants* on all surfaces. Clean all sides of each upholstered section. Follow the directions on the disinfectant and wipe off excess.

Recommended Disinfectants

Protex, MadaCide, Accell TB, Virox®

Note: Damage caused by unapproved substances will not be covered under the warranty.

DO NOT use citrus based cleaners or other strong cleaners, such as alcohol, acetone, higher concentrations of bleach or other products that contain high concentrations of these substances.

DO NOT expose the fabric to temperatures below 50°F/10°C or above 104°F/40°C.

DO NOT expose the fabric to direct sunlight, adhesives, liquids, or abrasive materials.

INSPECTIONS & MAINTENANCE

RECOMMENDED REGULAR INSPECTIONS (monthly or local standard)

- Check for damage to the power, hand control or foot control cables.
- Visually inspect components for obvious damage that could cause problems during operation.

RECOMMENDED PERIODIC INSPECTIONS (yearly or local standard)

- Check for damage to the power, hands control or foot control cables and all visible wiring.
- Visually inspect components for obvious damage that could cause problems during operation.
- Check all mechanical functions using the hand control. Repeat using the foot control. Check for abnormal noises.
- Replace any missing or illegible labels.
- Check that all fasteners are present and fastened securely.
- Check table grounding.
- Clean unusual buildup of dirt on the chair and/or parts of the chair not normally cleaned on a regular basis.
- Check for tears or cracks in the upholstery.

MAINTENANCE

- No specific maintenance tasks are required.
- Oakworks medical tables/chairs are designed and built to provide many years of dependable service. Please follow local regulations and laws when disposing of the electrical components used in this chair.
- ***For all Customer Service related problems refer to the Service Manual***

WARRANTY

View complete warranty details at www.oakworks.com

MODEL NUMBER & SERIAL NUMBER

MODEL & SERIAL NUMBERS




The model number and serial number are located on the frame of the top.

Model Numbers and Serial Numbers always start with a letter.

MODEL NUMBER DESCRIPTION

FL DT RT 22 26 84 MG TT XX XX

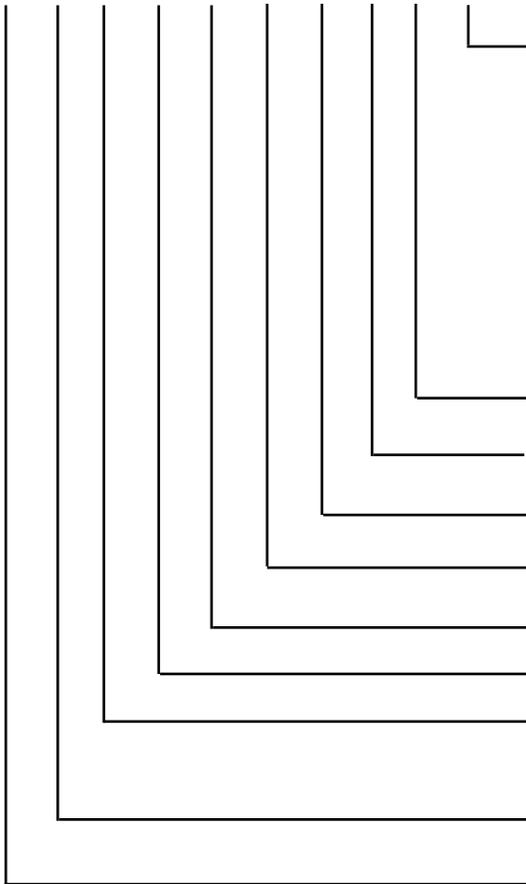

Options: May be in any order

- 5C = 5" (12.7 cm.) Casters
- 6L = 6" (15.2 cm.) T-Rail (Left Side)
- 6R = 6" (15.2 cm.) T-Rail (Right Side)
- 6B = 6" (15.2 cm.) T-Rail (Both Side)
- 2L = 20" (50.8 cm.) T-Rail (Left Side)
- 2R = 20" (50.8 cm.) T-Rail (Right Side)
- 2B = 20" (50.8 cm.) T-Rail (Both Side)
- 7L = 78" (198.1 cm.) T-Rail (Left Side)
- 7R = 78" (198.1 cm.) T-Rail (Right Side)
- 7B = 78" (198.1 cm.) T-Rail (Both Side)

Spaces not used

Fabric: TerraTouch™

Padding: Comfort Foam

Table Top Length

Minimum Table Height

Table Top Width

Top: Polycarbonate

RT = Rectangular

Base Motion: Dual Tower

Fluoroscopy Table

SPECIFICATIONS

PRODUCT SPECIFICATIONS	
Materials of Construction	This product contains no latex.
Top Frame	Extruded aluminum with powdercoated or anodized surfaces.
Table Top	.5" (1.3 cm.) Polycarbonate
Patient Comfort	1" (2.5 cm.) upholstered foam pad
Table Length	78" (198 cm.)
Table Width	24" (61 cm.)
Height Range	24"-40" (61-102 cm.) standard
Table Top Travel Range	±11.5" (29 cm)
Trendelenburg Tilt	±14°
Weight	390 lbs. (177 kg.)
Shipping Weight	526 lbs. (239 kg.)
Lifting Capacity	450 lbs. (205 kg.)
Aluminum Filtration Equivalent of Table top	TABLE TOP 100 kvp, Hvl of 3.6 mm = 1.62 (1.74 max)
	1" (2.5 cm.) TABLE TOP PAD 100 kvp, Hvl of 3.6 mm = .88 (1.07 max)
	2" (5 cm.) TABLE TOP PAD 100 kvp, Hvl of 3.6 mm = 1.47 (1.76 max)

This product complies with the United States Department of Health and Human Services radiation performance standards, 21 CFR Subchapter I, in effect at the time of manufacture for radiographic tables.

ENVIRONMENTAL CONDITIONS			
Conditions	Temperature	Humidity	Atmospheric Pressure
Normal Use	50° (10°C) to 104° (40°C)	20% to 60% RH	98 to 105 kPa
Storage & Transport	-20° (-29°C) to 135° (57°C)	20% to 95% RH	98 to 105 kPa

ELECTRICAL SPECIFICATIONS			
Designed for:	North America	Europe	Japan
Input Service	120 VAC/15 amp/60 Hz	220 VAC/10 amp/50/60 Hz	100 VAC/20 amp/50 Hz
Current Draw	5.8 amps	2.9 amps	4.8 amps
Maximum Momentary Current Consumption	6.0 amps	3.0 amps	7.2 amps
Voltage Output to Actuators	24 VDC	24 VDC	24 VDC
Electric Shock Protection	Class 1 Equipment	Class 1 Equipment	Class 1 Equipment
Tabletop Applied Part	 Type B Applied Part	 Type B Applied Part	 Type B Applied Part
Ingress Protection Rating	IPX0	IPX0	IPX0
Made of Operation	Intermittent Operation MAX 2 minutes ON 18 minutes off	Intermittent Operation MAX 2 minutes ON 18 minutes off	Intermittent Operation MAX 2 minutes ON 18 minutes off

SPECIFICATIONS

Guidance and Manufacturer's Declaration - Electromagnetic Emissions

The table is intended for use in the electromagnetic environment specified below. The customer or the user of the table should assure that it is used in such an environment.

Emissions Test	Compliance	Electromagnetic environment - guidance
RF emissions CISPR 11	Group 1	The table uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR 11	Class A	The table is suitable for use in all establishments other than domestic and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
Harmonic emissions IEC 61000-3-2	Class A	
Flicker emissions IEC 61000-3-3	Complies	

Recommended Separation Distances

between the portable and mobile RF Communications equipment and the table

The table is intended for use in the electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the table can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the table as recommended below, according to the maximum output of the communications equipment.

Rated maximum output power of transmitter W	Separation distance according to frequency of transmitter (m)		
	150 kHz to 80 MHz $d = 1.2 \sqrt{P}$	80 MHz to 800 MHz $d = 1.2 \sqrt{P}$	800 MHz to 2.5 GHz $d = 2.3 \sqrt{P}$
0.01	0.12	0.12	0.23
0.1	0.38	0.38	0.73
1	1.2	1.2	2.3
10	3.8	3.8	7.3
100	12	12	38

For transmitters rated at a maximum output power not listed above, the recommended separation distance d in meters (m) can be estimated using the equation applicable to the frequency of the transmitter, where P is maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

NOTE 1 At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

SPECIFICATIONS

Guidance and manufacturer's declaration - electromagnetic immunity

The table is intended for use in the electromagnetic environment specified below. The customer or the user of the table should assure that it is used in such an environment.

Immunity Test	IEC 60601 test level	Compliance level	Electromagnetic environment - guidance
Electrostatic discharge (ESD) IEC 61000-4-2	±6 kV contact ±8 kV air	±6 kV contact ±8 kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30 %.
Electrical fast transient/burst IEC 61000-4-4	±2 kV for power supply lines ±1 kV for input/output lines	±2 kV for power supply lines Not applicable	Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	±1 kV line(s) to line(s) ±2 kV line(s) to earth	±1 kV line(s) to line(s) ±2 kV line(s) to earth	Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	<5 % UT (>95 % dip in UT) for 0,5 cycle 40 % UT (60 % dip in UT) for 5 cycles 70 % UT (30 % dip in UT) for 25 cycles <5 % UT (>95 % dip in UT) for 5 sec	<5 % UT (>95 % dip in UT) for 0,5 cycle 40 % UT (60 % dip in UT) for 5 cycles 70 % UT (30 % dip in UT) for 25 cycles <5 % UT (>95 % dip in UT) for 5 sec	Mains power quality should be that of a typical commercial or hospital environment. If the user of the table requires continued operation during power mains interruptions, it is recommended that the table be powered from an uninterruptible power supply or a battery.
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	3 A / m	3 A / m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.

NOTE U_t is the a.c. mains voltage prior to application of the test level.

SPECIFICATIONS

Guidance and manufacturer's declaration - electromagnetic immunity

The table is intended for use in the electromagnetic environment specified below. The customer or the user of the table should assure that it is used in such an environment.

Immunity Test	IEC 60601 test level	Compliance level	Electromagnetic environment - guidance
<p>Conducted RF IEC 61000-4-6</p> <p>Radiated RF IEC 61000-4-3</p>	<p>3 Vrms 150 kHz to 80 MHz</p> <p>3 V/m 80 MHz to 2,5 GHz</p>	<p>3Vrms</p> <p>3V/m</p>	<p>Portable and mobile RF communications equipment should be used no closer to any part of the table, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter.</p> <p>Recommended separation distance</p> $d = 1,2 \sqrt{P}$ $d = 1,2 \sqrt{P} \quad 80 \text{ MHz to } 800 \text{ MHz}$ $d = 2,3 \sqrt{P} \quad 800 \text{ MHz to } 2,5 \text{ GHz}$ <p>Where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in meters (m).</p> <p>Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey, ^ashould be less than the compliance level in each frequency range. ^b</p> <p>Interference may occur in the vicinity of equipment marked with the following symbol:</p> 

NOTE 1 At 80 MHz and 800 MHz, the higher frequency range applies.

NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

^a Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the table is used exceeds the applicable RF compliance level above, the table should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as re-orienting or relocating the table

^b Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.

THIS PAGE IS INTENTIONALLY LEFT BLANK

USER MANUAL

OAKWORKS® DTPM300 Imaging Table

CONTACT INFORMATION:

OAKWORKS® Inc.

923 East Wellspring Road
New Freedom, PA 17349

Phone: 717-235-6807

FAX: 717-235-6798

www.oakworksmed.com

EC	REP	EMERGO EUROPE Molenstraat 15 2513 BH, The Hague The Netherlands
-----------	------------	---



Intertek

3034177

CONFORMS TO:
ANSI/AAMI STD ES60601-1
IEC STD 60601-1 3RD EDITION
IEC STD 60601-1-2 3RD EDITION
IEC STD 60601-1-6 3RD EDITION
IEC STD 60601-2-32
CERTIFIED TO CAN/CSA STD C22.2 NO. 60601-1
CB TEST CERTIFICATE AND REPORT

Manual Part Number MMMNST0017

Revision level: A

1st Edition, April 2010
2nd Edition, August 2013

English, Printed in USA

